



Axial3D Insight Operator Manual - QIH

IFU-OPS-006

Version 2

Table of contents

| | |
|--|----------|
| Table of contents | 2 |
| 1. Description of Axial3D Insight | 5 |
| 2. Indications for use | 5 |
| 3. Contraindications | 5 |
| 4. Cautions and warnings | 5 |
| 5. Validation of 3D printed models | 7 |
| 6. Instructions for use | 7 |
| 6.1. How to Register an Account on Axial3D Insight | 7 |
| 6.2. How to place an order - Uploading DICOM images Now | 8 |
| 6.2.1. Specialism/Anatomical Region(s) | 8 |
| 6.2.2. Patient Details | 8 |
| 6.2.3. Patient Pathology | 9 |
| 6.2.4. Model Type | 9 |
| 6.2.5. Date Required (optional) | 11 |
| 6.2.6. Upload DICOM Files | 11 |
| 6.2.6.1. Drag and drop | 11 |
| 6.2.6.2. Add Files | 11 |
| 6.2.6.3. Add Folder | 12 |
| 6.2.6.4. Refer upload to PACS Department | 12 |
| 6.2.7. Additional Requirements | 13 |
| 6.2.8. Order Summary and Place Order | 13 |
| 6.2.9. Email confirmation | 14 |
| 6.3. Uploading DICOM images later | 14 |
| 6.4. PACS image transfer request | 15 |
| 6.5. Uploading DICOM images later - Refer to PACs | 15 |
| 6.6. Adding additional DICOM images to order | 15 |
| 6.7. PACS Image Transfer | 16 |
| 6.8. How to Request a model - predefined order specification | 16 |
| 6.8.1. Enter Patient details | 17 |
| 6.8.2. Date Required (optional) | 17 |
| 6.8.3. Upload DICOM Files | 17 |
| 6.8.3.1. Drag and drop | 18 |

| | |
|--|-----------|
| 6.8.4. Add Files | 18 |
| 6.8.5. Add Folder | 18 |
| 6.8.6. PACS Image Transfer | 19 |
| 6.9. Exit Order Creation | 19 |
| 6.10. My Orders page | 19 |
| 6.11. List of validated printers | 20 |
| 7. Account Management | 26 |
| 7.1. Searching for an order on Axial3D Insight | 26 |
| 7.2. Changing accounts details | 26 |
| 7.3. Forgotten password | 26 |
| 7.4. Accessing Axial3D contact details | 27 |
| 7.5. Configure PACS Emails | 27 |
| 7.6. Log Out of platform | 27 |
| 7.7. Enabling custom order ID | 28 |
| 8. End user - receiving a 3D printed model from Axial3D | 28 |
| 9. End users receiving a Digital File | 28 |
| 10. End users - Printing a digital file | 29 |
| 11. Anatomical models printed on Stratasys Polyjet printer | 30 |
| 12. Anatomical models printed on Stratasys Origin One printer | 32 |
| 13. Anatomical models printed on HP printers | 35 |
| 14. Post-print visual check and reprinting or failed prints | 37 |
| 14.1. Formlabs Printer cleaning after failed print | 37 |
| 14.2. HP Printer cleaning after failed print | 37 |
| 14.3. Stratasys Polyjet Printer cleaning after failed print | 37 |
| 14.4. Stratasys Origin One Printer cleaning after failed print | 38 |
| 14.5. Post-processing 3D printed models | 38 |
| 14.5.1. Formlabs post-processing of 3D models - Removing parts from the build platform | 38 |
| 14.5.1.1. Drying parts | 39 |
| 14.5.1.2. Removing support structures | 39 |
| 14.5.1.3. Post curing prints using a Form Cure | 41 |
| 14.5.2. Form Cure material settings: | 43 |
| 14.5.3. Removing Support Bumps from 3D Models | 44 |
| 14.6. HP post-processing of 3D printed models | 46 |
| 14.7. Stratasys post-processing of 3D printed models on Polyjet technology | |

| | |
|--|-----------|
| 47 | |
| 14.8. Stratasys post-processing of 3D printed models on DLP technology | 48 |
| 14.9. Final inspection of the 3D printed model | 49 |
| 15. Symbols glossary | 50 |
| 16. Manufacturer details | 52 |
| 17. Reporting to adverse events to the FDA | 53 |
| 18. Glossary | 55 |
| 19. Appendix Axial3D Insight Release Notes v2.0.0 | 59 |
| 19.1. Known Software Anomalies | 59 |

1. Description of Axial3D Insight

Axial3D Insight is a secure, highly available cloud-based image processing, segmentation and 3D modeling framework for the transfer of imaging information to either a digital file or as a 3D printed physical model.

Axial3D Insight is made up of a number of component parts, which allow the production of patient-specific 1:1 scale replica models, either as a digital file or as a 3D printed physical model.

2. Indications for use

Axial3D Insight is intended for use as a cloud-based service and image segmentation framework for the transfer of DICOM imaging information from a medical scanner to an output file.

The Axial3D Insight output file can be used for the fabrication of physical replicas of the output file using additive manufacturing methods.

The output file or physical replica can be used for treatment planning. The output file or physical replica can be used for diagnostic purposes in the field of trauma, orthopedic, maxillofacial and cardiovascular applications.

Axial3D Insight should be used in conjunction with other diagnostic tools and expert clinical judgment.

3. Contraindications

Axial3D Insight is not intended for use with Ultrasound and X-Ray imaging.

4. Cautions and warnings

Axial3D Insight is intended for use by trained medical professionals for surgical planning in the following applications: trauma, orthopedics, maxillofacial, and cardiovascular.



The physical 3D printed model or digital file should be used in conjunction with expert clinical judgment and alongside the original DICOM images. Changes in patient anatomy may occur between the time of imaging and surgery, this may impact the performance of the 3D printed physical model, the patient should be assessed for changes in anatomical structures prior to the procedure.

The 3D printed physical models are not intended for sterilization or for use within a sterile field.

Fragments present in orthopedic models below 5 mm shall be removed from the digital file to be printed, this is to reduce the risk of these fragments breaking away from the model during post-processing practices

Users intending to 3D print digital files provided by Axial Medical Printing Limited must be able to follow post-processing and inspection guidelines provided by Axial Medical Printing Limited to ensure the diagnostic quality of the anatomical model. If these processes are not followed, the diagnostic quality of the final 3D printed physical model cannot be guaranteed.

Axial3D defines trauma as orthopedic trauma and craniomaxillofacial trauma including complex fractures in which the 3D images and associated physical models would be used for surgical planning. Fragments present in orthopedic trauma and craniomaxillofacial trauma models below 5mm shall be removed from the digital file to be printed, this is to reduce the risk of these fragments breaking away from the model during post-processing practices.

Please ensure that you are using the latest version of the supported browsers, and you have antivirus protection installed on your end user device. To access the service, all communication is via HTTPS, and only port 443 is required to be open. Any issues with the service will be communicated to you via your registered email address.

5. Validation of 3D printed models

The validation of the physical printed models was completed by CT scanning the physical 3D printed model with a 0.67 mm slice spacing on the Philips Brilliance iCT 256 CT Scanner and compared with the original DICOM data. The Philips machine used in the validation testing is the following FDA cleared device:

Name: System, X-Ray, Tomography, Computed

Product Code: JAK

Regulation No: 21 CFR 892.1750

Class: 11 Panel: Radiology

6. Instructions for use

6.1. How to Register an Account on Axial3D Insight

- Visit <https://orders.axial3d.com/login>
- Click on Register a new account
- Enter all information requested on page:
 - **Title**
 - **First Name**
 - **Last Name**
 - **Email**
 - **Telephone Number (Optional)**
- **Password** (Requires at least 8 characters with at least 1 letter, 1 number, and 1 special character)
- **Confirm Password** (must match previous Password Entry)
- Click the Box to **Accept Axial3D Terms of Use and Privacy Policy** (Click on Terms of Use and Privacy Policy to read)
- Click **Submit** to complete registration.
- The next page will provide the following message:



Email Confirmation

Thank you for signing up.

Please check your email and click on the Account Confirmation link sent to yourname@email.com This link will expire in 24 hours.

Once you have confirmed your account, you can Login.

[Go to Login button]

Need help setting up your account? Call us on +1 857 412 7244 (US) / +44(0)28 9018 3590 (UK/EU) or email us at orders@axial3d.com

6.2. How to place an order - Uploading DICOM images Now

- Login with registered account details at <https://orders.axial3d.com/login>
- Click **New Order** to request a 3D model

6.2.1. Specialism/Anatomical Region(s)

- Choose a **Specialism/Anatomical Region** from the drop menu
- Choose a **Sub Region(s)** from the drop down menu to specify anatomy required
 - Select either **Oncology and/or Trauma** (optional) if relevant to the patients pathology

6.2.2. Patient Details

- Provide **Custom Order ID (optional)**, this ID is specific to customer internal records
 - To enable this feature reference [Section 7.7 Enabling Custom Order ID](#)
- Provide patient **Birth Year** if unknown select **Undisclosed** from dropdown
- Provide **Gender** if unknown select **Undisclosed** from dropdown

6.2.3. Patient Pathology

- Provide details of the **anatomical structures** needed in the model
 - List all specific areas required
- Provide details of the **patients relevant pathology**
 - Provide a brief description of the patients condition or diagnosis
- If the selected specialism is Orthopaedic, Neurology or CMF specialism, select if you would like to include any **implants or foreign bodies** visible in the scan in the final 3D model. Or, select 'N/A' if not applicable
- If the selected specialism is Cardiothoracic & Vascular, and you know what **type of cuts** you require on the model, please select from the drop down options.
 - Select **Add Cut** and choose **Cut Type** and **Cut Location** from the drop down menu. Multiple cuts can be added.
 - If the desired cuts are unknown, select **No**, and use the text box to describe the internal anatomy you would like to view.
- If the selected specialism is General surgery, Urology & Gynaecology or Other, no additional questions are required.

6.2.4. Model Type

- Choose **model type**
- Select from **digital model(s)**
 - **3D Visual**, included with all orders
 - **3D Mesh**
 - **3D Print-ready file**
- If a **3D Print-ready file** is selected, provide details of **3D Print-Ready Requirements**

- Specify your **printer model/size** (optional)
- Select a physical model
 - **3D Print**
- If a 3D Print is selected provide details of **3D Print Requirements**
- Select **model material**
 - **Standard:** suitable for visualizing the anatomy but can not be drilled
 - **Tissue Mimicking:** Suitable for case rehearsal, if you need to drill or cut bone models or suture cardiac models
 - **Not Sure:** the Axial3D team will contact you to help determine the most appropriate material
- Add **3D Print Delivery Details**
 - Select **Add an Address** to enter the details for shipping
 - Returning customers can select a previously entered address from the dropdown menu, or select **Add an Address** to enter a new location

6.2.5. Date Required (optional)

- This is an optional field. If you don't need your order right away, you can choose a later delivery date. If no date is selected, we will deliver as soon as possible.

6.2.6. Upload DICOM Files

- DICOM files can be uploaded by either dragging and dropping the images into the upload window, selecting the DICOM files to upload, selecting the DICOM folder to upload or referring the upload process to the PACS Department.

6.2.6.1. Drag and drop

- Open the folder on your computer (or disk) where the files are located
- **Highlight all DICOM images (.dcm)**
 - Do not include the DICOM viewer
 - We also accept compressed ZIP format folders of .dcm files
 - We do not accept files that are not .dcm
- Drag the files onto the order screen in the area marked **Drag and Drop to Upload Files**
 - You can confirm the number of files matches at the right of your screen in the summary

6.2.6.2. Add Files

- Select **Add Files**
- Navigate to the DICOM images on your computer (or disk) where the files are located
- Select all images in the DICOM folder
- Select Open

6.2.6.3. Add Folder

- Select **Add Folder**
- Navigate to the folder containing all DICOM images on your computer (or disk) where the folder is located. The folder must be a compressed zipped folder to upload
 - Only upload DICOM images associated with the patient in the order details. Each upload should only contain scans for one patient.
 - Do not upload images for multiple patients into one order.
- Select the relevant folder
 - Select **Open**
- This process can be repeated if more DICOM files are available to upload
- If the DICOMs are not available at the time of placing the order, the rest of the order details can be completed, the order can still be placed and the images can be uploaded at a later time. Complete as much of the order form as possible, then select **Place order**. If DICOM images are missing, a popup message will appear before placing the order to highlight this. Click **No, go back** if you do have access to the images and want to upload now, or click **Yes, upload later** if you will access to the images at a later time. [Section 6.3 Uploading DICOM images later](#) provides instructions for uploading images at a later time.

6.2.6.4. Refer upload to PACS Department

- Select **Refer upload to PACS Department**
- **Request a scan from your PACS Department**, select an email from the drop-down menu
- If the required email address is not available in the drop-down menu, select **Add a new email**
 - Enter the name and email for the PACs contact

Note: If this is a new email address, you must select **Add Contact** to proceed with the PACs referral

- Enter the **Patient Healthcare ID**
- Enter **Scan type(s)**, e.g. CT or MRI
- Enter **Scan date**
- Provide additional information in the **Scan notes** if required for the PACS department
- If the patient has more than one scan that is required for the order, select **Add another scan to this request**
 - Enter **the Scan type(s)**
 - Enter **Scan date**
 - Enter **Scan Notes**
 - For PACS Departments uploading images on a requesters behalf, follow [Section 6.7 PACS Image Transfer](#)

6.2.7. Additional Requirements

- This is an optional field. Please include any additional requirements or comments for processing the order here.

6.2.8. Order Summary and Place Order

- Order details can be reviewed to ensure all details are correct. Once reviewed, select **Place Order**
- If a section has not been completed, the **Order Summary** will identify the information to be provided before completing the order
- Once the order is placed, the DICOM files will be uploaded to the order
- A notification will appear to confirm that the order is complete
 - Select **Create Another Order** to create a new order
 - Select **Copy Order** if another model is required with the same requirements
 - Select **View My Orders** to return to the **My Orders** page

6.2.9. Email confirmation

- An email will be sent to the address registered on the ordering platform.
- The email will confirm order specifications, and contain a reference to the order number.
- Select **View Order** to open the order within the Insight platform
- The order will also be accessible from the table accessed at **My Orders** from the main menu

6.3. Uploading DICOM images later

- Login with registered account details at <https://orders.axial3d.com/login>
- On the **My Orders** page, navigate to the order number that requires DICOM files
- If DICOM files are required, this will be highlighted on the order
- Select **Add Files**
- DICOM files can be uploaded by either dragging and dropping the images into the upload window, selecting the DICOM files to upload or selecting the DICOM folder to upload.
 - Follow [Section 6.2.6 Upload DICOM Files](#) for further details
- Once the files have been added, select **Start Upload** to complete the upload of DICOMs to the order
- Ensure upload is complete before closing webpage
- Select **Upload More DICOMs** if more DICOM files can be added to the order

6.4. PACS image transfer request

Image transfer options are available for PACs/Imaging departments. Images can be transferred securely to Axial3D via IEP and Powershare Networks. Contact Axial3D for more information on setting up a secure image transfer connection. *Call us on +1 857 412 7244 (US) / +44(0)28 9018 3590 (UK/EU) or email us at orders@axial3d.com*

6.5. Uploading DICOM images later - Refer to PACs

- Login with registered account details at <https://orders.axial3d.com/login>
- On the **My Orders** page, navigate to the order number that requires DICOM files
- If DICOM files are required, this will be highlighted on the order
- Select **Add Files**, this will open the order details page
- Select **Refer to PACs** from the drop-down menu
 - Reference [Section 6.2.6.4 Refer upload to PACs Department](#)

6.6. Adding additional DICOM images to order

Additional DICOM images can be added after the order has been placed, and after the initial DICOMS have been uploaded.

- Login with registered account details at <https://orders.axial3d.com/login>
- On the My Orders page, navigate to the order number that requires additional DICOM files
- Click on the order to open the order details page
- To upload files directly to the order, select Add DICOMS
- Reference Section [6.2.6.1](#), [6.2.6.2](#), [6.2.6.3](#) above for details on how to complete this
- To upload files via PACs transfer, select Refer to PACs
- Reference [Section 6.2.6.4](#) above for details on how to complete this

6.7. PACS Image Transfer

- This section is relevant to those in PACs imaging department who will be transferring images to Axial3D on behalf of someone else
- Click on the **Transfer Files** button in your email request you received from orders.axial3d.com
 - Note: This transfer link expires 72 hours following request
- Your Web Browser will open up to an **Axial3D page** to upload imagesRegistration and login is not required for PACS team member to upload files
 - Follow [Section 6.2.6.4 Refer upload to PACs Department](#) for further details
- Click **Start Upload** (once you confirm you have the correct number and type of files)
 - The upload screen will provide the progress of the upload
 - When completed, the Upload Progress will be 100% and a message will display saying **Upload Successful** for order number (RC)PXXXXX
 - If you wish to upload more DICOMs, select **Upload More DICOMs** and repeat the upload process

6.8. How to Request a model - predefined order specification

Customers who request the same model type for each patient case will have a list of predefined orders to select from.

- Login with registered account details at <https://orders.axial3d.com/login>
- Select **New Order**
- Select **Predefined Order**

- From the drop-down select the Predefined Order Type required for the patients case, e.g. Hip - 3D Visual/3D Mesh
- Enter **Custom Order Requirements (Optional)**, this optional field can be populated with additional information if the model requested requires minor customizations to the standard order requirements. Specify all modifications in this field.

6.8.1. Enter Patient details

- **Custom Order ID** (optional), this ID is specific to customer's internal records
 - To enable this feature reference [Section 7.7 Enabling Custom Order ID](#)
 - Patient **Birth Year**
 - Patient **Gender**

6.8.2. Date Required (optional)

- This is an optional field. If you don't need your order right away, you can choose a later delivery date. If no date is selected, we will deliver as soon as possible

6.8.3. Upload DICOM Files

- DICOM files can be uploaded by either dragging and dropping the images into the upload window, selecting the DICOM files to upload, or selecting the DICOM folder to upload or referring the upload process to the PACS Department.

6.8.3.1. Drag and drop

- Open the folder on your computer (or disk) where the files are located
- Highlight all DICOM images (.dcm)
 - Do not include the DICOM viewer
 - We also accept compressed ZIP format folders of .dcm files
 - We do not accept files that are not .dcm
- Drag the files onto the Screen in the area marked **Drag and Drop to Upload Files**
 - You can confirm the number of files matches at the right of your screen in the summary

6.8.4. Add Files

- Select Add Files, and navigate to the DICOM images, select all images in the DICOM folder and select Open

6.8.5. Add Folder

- Select **Add Folder**, and navigate to the folder containing all DICOM images. The folder must be a compressed zipped folder to upload
 - Only upload DICOM images associated with the patient in the order details. Each upload should only contain scans for one patient; do not upload images for multiple patients into one order.
- This process can be repeated if more DICOM files are available to upload
- If the DICOMs are not available at the time of placing the order, the rest of the order details can be completed, and the images can be uploaded at a later time. [Section 6.3 Uploading DICOM images later](#) provides instructions for uploading images at a later time.

6.8.6. PACS Image Transfer

- This section is relevant to those in PACS imaging department who will be transferring images to Axial3D on behalf of someone else
- Click on the **Transfer Files** button in your email request you received from orders.axial3d.com
 - Note: This transfer link expired 72 hours following request
- Your Web Browser will open up to an **Axial3D page** to upload images, registration and login is not required for PACS team member to upload files
- Follow [Section 6.2.6.4 Refer upload to PACS Department](#) for further details

6.9. Exit Order Creation

The order can be cancelled at any time during the ordering process. Select Exit Order, to return to the **My Orders** page

6.10. My Orders page



- Login with registered account details at <https://orders.axial3d.com/login>
- By default, this will open on **My Orders**
- All order requests can be viewed on **My Orders** page, this will display
 - Order Date
 - Order ID/ Custom Order ID
 - Patient info
 - Specialism/Anatomical Region
 - Files : Number of Files processed and Number of Valid DICOMs

- Order Type, 3D Visual, 3D Mesh, Print ready File, 3D Print
- Order Status
- Order Status will automatically update as the order progresses through production.
- If the Order Status appears in Red there is an action required of the Order Requester
 - **DICOMs required:** The Order request has not received DICOMs, the processing will not commence on the order until valid DICOM have been received. Follow [Section 6.2.6 Upload DICOM Files](#)
 - **Awaiting Approval:** 3D visual has been sent to the requestor to approve, before production will continue.
 - The 3D visual can be reviewed in the order
 - Select the order number that has an associated approval action
 - The 3D visual will appear on the screen to review
- Email the Axial3D team to approve the order or request further edits

6.11. List of validated printers



The following printers and materials have been validated for 3D printing anatomical models.



NOTE: Using other printers or materials will require additional validation and testing.

| Printer Manufacturer | Technology | Model | Material | Applications |
|----------------------|--------------------|---|-------------------------------|--|
| Formlabs | Vat Polymerization | Form 3B | Standard White V4 FLGPWH04 | Orthopedics Cardiovascular Maxillofacial |
| | | Form 3L | | |
| | | Form 3BL | | |
| | |  | Standard Draft V2 FLDRGR02 | Orthopedics Maxillofacial Cardiovascular |
| | | | Standard Clear V4 FLGPCL04 | Cardiovascular |
| | | | Flexible 80A V1 FLFL8001 | Cardiovascular |
| | | | Standard Clear V4.1 | Cardiovascular |
| | |  | Biomed White Resin | Orthopedics Cardiovascular Maxillofacial |



| | | | | |
|--|--|--|--------------------|----------------|
| | | | Biomed Clear Resin | Cardiovascular |
|--|--|--|--------------------|----------------|

Note: BioMed White and BioMed Clear material can only be printed on Form 3B and Form 3BL

| Printer Manufacturer | Technology | Model | Material | Applications |
|----------------------|------------|---|---|--|
| Stratasys | Polyjet | J750  | Agilus, VeroBlackPlus, VeroClear, VeroCyan, VeroGrey, VeroMagenta, VeroPureWhite, VeroYellow | Orthopedics Cardiovascular Maxillofacial |
| | Polyjet | J5 MediJet  | VeroVividTM Cyan, VeroVividTM Magenta, VeroVividTM Yellow, DraftWhite, MED610, MED615RGD, VeroUltraClearTM , ElasticoTM Clear | Orthopedics Cardiovascular Maxillofacial |

| | | | | |
|--|---------|---|--|--|
| | Polyjet | J850  | VeroVivid™ Cyan, VeroVivid™ Magenta, VeroVivid™ Yellow, VeroPureWhite BoneMatrix™ GelMatrix™ TissueMatrix™ RadioMatrix™ Agilus30 VeroClear VeroMagenta BlackPlus | Orthopedics Cardiovascular Maxillofacial |
| | DLP | Origin One  | LOCTITE 3D 3172 ORIGIN DM100 by BASF ORIGIN DM200 by BASF LOCTITE 3D 3843 LOCTITE 3D IND405 | Orthopedics Cardiovascular Maxillofacial |

Note: Anatomical 3D printed models have not been validated for printing in a combination of materials with differing physical properties

| Printer Manufacturer | Technology | Model | Material | Applications |
|----------------------|------------------|--|------------|--|
| HP | Multi-jet Fusion | HP580  | Nylon PA12 | Orthopedics Cardiovascular Maxillofacial |
| | Multi-jet Fusion | HP540  | Nylon PA12 | Orthopedics Cardiovascular Maxillofacial |

7. Account Management

7.1. Searching for an order on Axial3D Insight

- Login with registered account details at <https://orders.axial3d.com/login>
- By default, this will open on **My Orders**
- Scroll down through orders presented on the **My Orders** table
- Or Enter (RC)PXXXXX in **Search order number** field (this will bring up that specific order)

7.2. Changing accounts details

- Login with registered account details at <https://orders.axial3d.com/login>
- Click **Account**
- Click **Change Password**
- Enter **Current Password**
- Enter **New Password**
- Click **Update**

7.3. Forgotten password

- Visit <https://orders.axial3d.com/login>
- Click **Reset your password**
- Enter **Email Address**
- Click **Continue**
- Select **Reset password** via the email link you will receive from Axial3D in your Inbox

- Enter **New Password**
- Confirm **New Password**
- Click **Submit**

7.4. Accessing Axial3D contact details

- Login with registered account details at <https://orders.axial3d.com/login>
- Click **Account**
- Click **Support**

7.5. Configure PACS Emails

- Login with registered account details at <https://orders.axial3d.com/login>
- Select **Account**
- Select **Configure PACS Emails**
- Add new PACS email contact, enter **Name** and **Email** of PACS contact
- Select **Add Contact**
- Additional PACS contacts will be available from the drop-down menu when requesting a PACS transfer [Section 6.2.6.4](#)

7.6. Log Out of platform

- Click **Account**
- Select **Sign Out**

7.7. Enabling custom order ID

If a custom ID is required on the model, this feature must be enabled within account management settings

- Login with registered account details at <https://orders.axial3d.com/login>
- Navigate to **Account**
- Select **Order Options**
- Select **Enable Custom Order ID in order creation**
- Select **Save**

8. End user - receiving a 3D printed model from Axial3D

On completion of the end users order request, Axial3D engineer will process the DICOM images to produce a digital file for printing. Axial3D engineer will 3D print the anatomical model on their validated printers. The end user will receive an automated email notification that their 3D printed model has been dispatched. The completed 3D model will be delivered to the delivery address provided by the end user.

9. End users receiving a Digital File

On completion of an Axial3D engineer processing an order to produce a digital file, an automated email will be sent to the end user to advise that the digital file is ready to be downloaded. The end user can retrieve the digital by following the steps outlined below

- Login with registered account details at <https://orders.axial3d.com/login>
- Select **My Orders**
- Navigate to the order number by entering (RC)PXXXXX in **Search order number** field, or by scrolling down through orders presented on the **My Order** table
- Click into the relevant order
- Click **Download 3D Product Files**

- A zip file will automatically download containing the digital file(s)
- Note: To review and use the 3D product files, please extract them from the .zip folder first.

10. End users - Printing a digital file

Axial3D has validated the printing of digital files on the list of 3D printers identified in [Section 6.11. List of validated printers](#). An end user that receives a digital file can upload the digital file to the validated 3D printer, using the manufacturer's print file generation software, to produce a physical 3D printed anatomical model. The end user must be trained by the printer manufacturer or a qualified 3D printer technician within their facility on the process for 3D printing models.

The end user intending to 3D print digital files provided by Axial3D must be able to follow the below guidelines on uploading a digital file to the printer, post-processing, and inspection guidelines provided by Axial3D, to ensure the diagnostic quality of the anatomical model. If these processes are not followed the diagnostic quality of the final 3D printed physical model cannot be guaranteed.

The end user can upload the digital file to the 3D printer manufacturer's print file generation software. Below is the recommended software.

| Printer Manufacturer | Printer Model | Software |
|----------------------|------------------------------------|----------|
| Formlabs | Form 2, Form 3B, Form 3L, Form 3BL | PreForm |
| Stratasys | J750, J5, J850 | GrabCAD |

| | | |
|-----------|--------------|---------------------------------|
| Stratasys | Origin One | Netfabb and GrabCAD |
| HP | HP580, HP540 | HP SmartStream 3D Build Manager |

Anatomical models printed on Formlabs Form 3B, Form 3L and Form3BL printers must be printed in the following orientation for optimal print orientation layout. The end user must follow Axial3D validated print file orientation instructions. If these processes are not followed, the diagnostic quality of the final 3D printed physical model cannot be guaranteed.

- 3D model is angled at a 20 - 60 degree angle to decrease the amount of surface area in contact with the resin tank, which in turn reduces the amount of force on the 3D printed physical models as the build platform raises with each layer.
recommended procedures ref: *WI-OPS-062 Preform Setup for Form3& 3B - Customer instructions*
- Orient the model to stand with the merging feature facing toward the build platform to create a shared base for branching features to grow from. Instead of layers coming together at a joint, the layers separate into individual paths
- Overhanging features are oriented to self-support during the printing process
- The region of the model is elevated to be printed towards the mixer side to reduce the print time for the final layers of the model.
- Post-print processes should be followed in line with Axial3D recommended Procedures ref: *WI-OPS-063 Formlabs Post-processing - Customer instructions*

11. Anatomical models printed on Stratasys Polyjet printer

- Insert STL file in the default position (File→ Add models)
- Arrange the model in the tray with an auto arrangement set.
- Assign material and send to printer - recommended procedures ref: *WI-OPS-059*


- Polyjet GrabCAD Print Scene Generation - Customer Instructions

- Post-print processes should be followed in line with Stratasys recommended procedures *ref: WI-OPS-061 - J5 Post-processing - Customer Instructions; WI-OPS-060 - J850 Post-processing - Customer Instructions*

12. Anatomical models printed on Stratasys Origin One printer


LOCTITE 3D 3172 printed models

| | |
|------------------------------------|--------------------------------------|
| Best printing orientation | 20 degrees (Y-axis) |
| Best printing build plate position | Front Left hand side and back center |

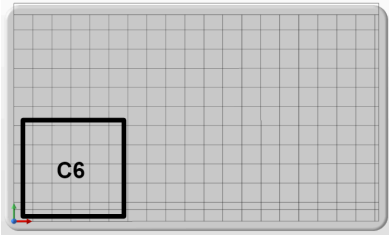

ORIGIN DM100 by BASF printed models


| | |
|------------------------------------|---|
| Best printing orientation | 0 degrees (XYZ-axis), 90 degrees (Y-axis) |
| Best printing build plate position | All locations on build plate |

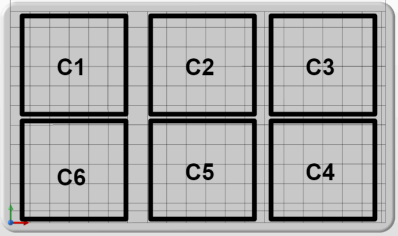

ORIGIN DM200 by BASF printed models

Best printing orientation 90 degrees (X-axis)


Best printing build plate position All locations on build plate

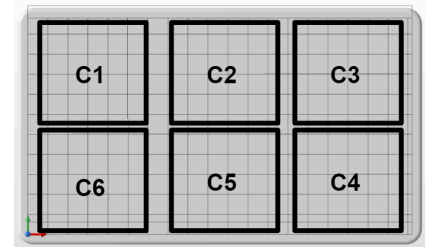

LOCTITE 3D 3843 printed models

Best printing orientation 0 degrees (XYZ-axis) (Flat to the build plate)


Best printing build plate position Back left

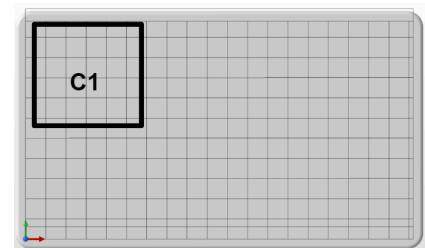

LOCTITE 3D IND405 printed models

Best printing orientation 20 degrees (Y-axis) / 0 degrees (XYZ-axis)

Best printing build plate position Back center and right position

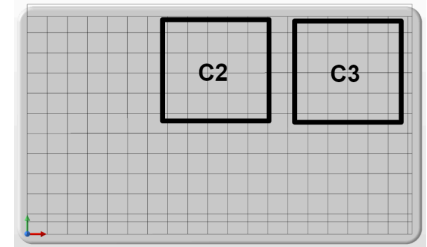

- The 3D model is angled between 0 - 90 degrees depending on material and geometry. Altering the angle will decrease the amount of surface area in contact with the resin tank, which in turn reduces the amount of force on the 3D printed physical models as the build platform raises with each layer. The optimal orientation will also limit the amount of support structures required during printing.
- Orient the model to stand with the merging feature of the geometry facing toward the build platform to create a shared base for branching features to grow from. Instead of layers coming together at a joint, the layers separate into individual paths. The optimal orientation from a branching point will also limit the amount of support structures required during printing.
- Overhanging features should be oriented to self-support during the printing process, where possible. This will in turn reduce post-processing times through less supports.
- All models to be printed in DLP need to be elevated 5mm from the build plate to ensure print success.
- Once the model is orientated at the optimal angle and elevated 5mm from the build plate the support generation function is ran.
- After support generation the supports are merged to the model and the print file is generated.

- The print file is then imported in to the printing software and the resin type is selected. The job is then uploaded to the Origin One printer and started.
- Post-print processes should be followed in line with Axial3D recommended procedures.

13. Anatomical models printed on HP printers

When parts are added, the application automatically checks that the parts satisfy various conditions:

- In bounds, ensuring parts are positioned within the build volume
- Closed mesh
- Correctly oriented, orient each part by placing its critical features on the horizontal XY-plane as this will provide the highest resolution.
- Place small features such as pins, holes, and thin walls upside-down on the XY plane to improve their look, feel, and strength. This also applies to raised texts, which should be printed on the XY-plane for maximum resolution
- Topologically valid: Are the parts printable? Parts beyond the boundaries of the build volume are considered out of bounds. Out-of-bounds parts can usually be fixed by clicking Auto-pack, or by manually moving the out-of-bounds part into the build volume. Parts with holes, troublesome orientations, and topologically invalid parts can be fixed by clicking Auto-Pack
- Remove the build unit from the printer after printing the parts
- Allow models to cool for the recommended time based on volume

| Build chamber | Printing time | | Safety cooling time | Natural cooling time | | Fast cooling time * |
|---------------|-----------------|-----------------------------|---------------------|----------------------|-----------|---------------------|
| | Fast print mode | Default/Strength print mode | | Normal | Minimum * | |
| 100% full | 10 h | 16 h 20 min | 20–30 min | 46 h | 31 h | 10 h |
| 75% full | 7 h 30 min | 12 h 15 min | 20–30 min | 35 h | 23 h | 8 h |

| Build chamber | Printing time | | Safety cooling time | Natural cooling time | | Fast cooling time * |
|---------------|-----------------|-----------------------------|---------------------|----------------------|-----------|---------------------|
| | Fast print mode | Default/Strength print mode | | Normal | Minimum * | |
| 50% full | 5 h | 8 h 10 min | 20–30 min | 23 h | 16 h | 6.5 h |
| 25% full | 2 h 30 min | 4 h | 20–30 min | 12 h | 8 h | 5 h |

- Once models have been cooled you must clean the parts to remove the thin layer of material attached to the surface.
- To do this, you need a bead-blasting machine. HP recommends a bead-blasting machine with the following specifications:
- Manual or automatic operation; Air pressure in the range 2–5 bar (29–72.5 psi); Glass beads of 70–110 µm diameter (0.00276–0.00433 in)
- This process consists of shooting an abrasive media, usually a bead (size and type results in different surface finishes), at high pressure at a printed part with compressed air, knocking loose unfused powder while also smoothing the finish of the part.

14. Post-print visual check and reprinting or failed prints

On completion of the 3D printing process at the end users facility a visual check of the printed model should be carried out to confirm that there are no defects. If a defect is identified the model should be reprinted. Before reprinting the end user should inspect and clean the 3D printer after a print failure, in line with the printer manufacturers guidelines.

14.1. Formlabs Printer cleaning after failed print

A failed print can result in small partially cured resin floating within the tank or stuck to the film at the bottom of the tank. Before a new print can be started the resin tank should be cleaned by the end user. It is advised that after each print the tank should be inspected to ensure it is clear of small resin particles or debris. To clean the tank the end user should follow the recommended guidelines provided by Formlabs on cleaning resin tanks. Once the resin tank has been cleaned the print can be restarted.

14.2. HP Printer cleaning after failed print

If a defect is detected on completion of the 3D print on the HP machine. It is recommended to clear the build chamber before a new print can be started. The end user should follow HP guidelines on cleaning and maintenance of HP printers. Once the printer has been inspected and cleaned the model can be reprinted.

14.3. Stratasys Polyjet Printer cleaning after failed print

If a defect is detected on completion of the 3D print on the Stratasys Polyjet machine, it is recommended to clear the build chamber before a new print can be started.. The end user should follow Stratasys guidelines on cleaning and maintenance of the printer. Once the printer has been inspected and cleaned the model can be reprinted.

If additional support is required the end user should contact **orders@axial3d.com** or call us on **+1 857 412 7244 (US) / +44 (0) 28 9018 3590 (UK/EU)**

14.4. Stratasys Origin One Printer cleaning after failed print

A failed print can result in small partially cured resin floating within the tank or stuck to the film at the bottom of the tank. Before a new print can be started the resin tank should be cleaned by the end user. It is advised that after each print the tank should be inspected to ensure it is clear of small resin particles or debris. To clean the tank the end user should follow the recommended guidelines provided by Stratasys on cleaning Origin One resin tanks. Once the resin tank has been cleaned the print can be restarted.


If additional support is required, the end user should contact **orders@axial3d.com** or call us on **+1 857 412 7244 (US) / +44 (0) 28 9018 3590 (UK/EU)**

14.5. Post-processing 3D printed models

3D printed anatomical models printed on the end users premises on their printing technology must be post-processed in line with the printer manufacturers guidelines. If these guidelines are not followed Axial3D cannot ensure the diagnostic quality of the final 3D printed model.

14.5.1. Formlabs post-processing of 3D models - Removing parts from the build platform

To remove the model from the build plate, ensure the snips are flat to the build plate. Snip around the base of the model. Once complete, using a rounded edge scraper, slide under the edges previously released by snips. This should allow the model to gently detach from the build plate.

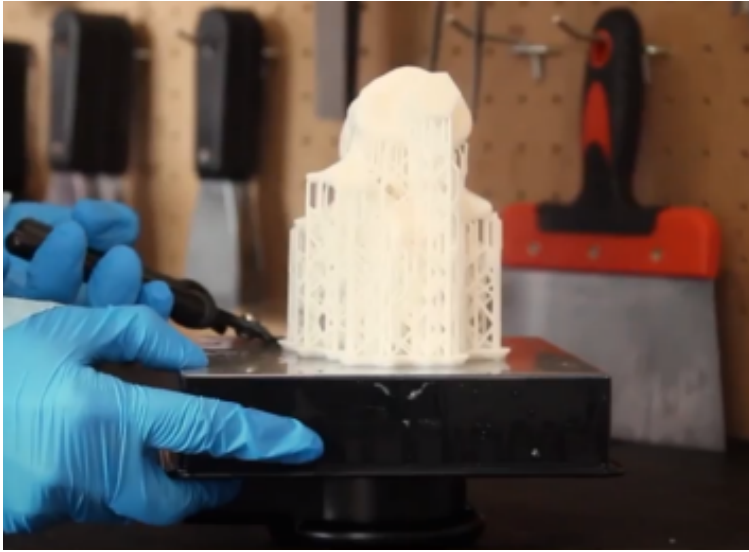

Carefully do this over a table to avoid the model dropping from a height. Using a round edged scraper to scrape off any excess left behind on the build plate. Scrape away from yourself.

Using some IPA and paper towels, wipe down the top surfaces as well as the edges of the build plate until all surfaces are free of resin.

NOTE: It is important to keep the printer and build plate clean so as to avoid any faulty prints in future. Always check the printer and build plates for cleanliness after every print. This can be done using clean IPA and paper towels.

14.5.1.1. Drying parts


Always let prints fully dry before placing them in the Form Cure to avoid the models becoming tacky. Microfiber cloths can be used to dry the excess IPA on the model. Allow parts to dry for at least 30 minutes after washing to allow the solvent to fully evaporate from part surfaces. Ensure the area is highly ventilated while the solvent evaporates.

14.5.1.2. Removing support structures


Using wire snips, cut around the base to break the raft into smaller sections.

Using a large sharp-edged scraper and cutting through the support next to the base to fully remove the raft.

Ensure to take great care using the large scraper to remove the raft from the model.

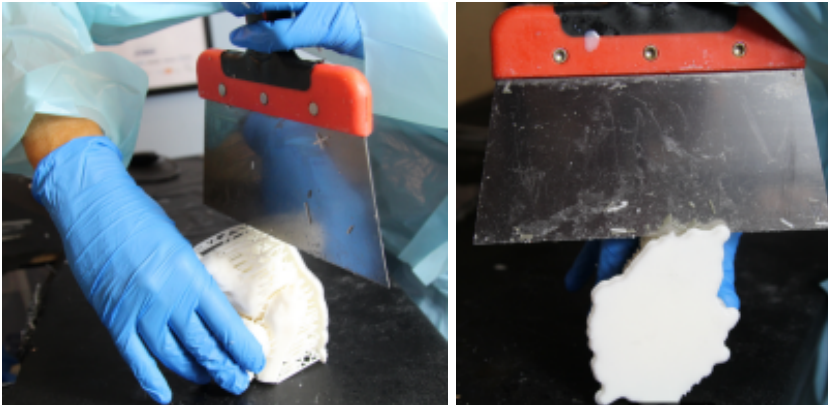

Use the wire snips to slowly release the supports from the model, breaking off small sections until complete.

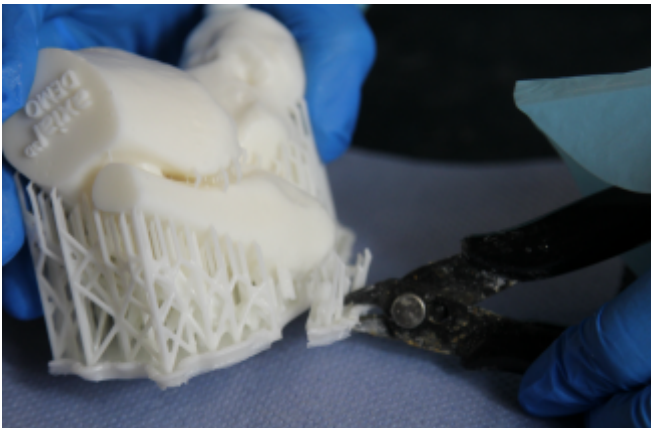

Carefully remove supports from delicate areas, use light pressure when snipping. Cut from the bottom of the support moving closer to the surface to avoid breaking off small features.

Small hand files and tweezers can be used for highly detailed parts. If parts still feel too fragile to remove supports, place into FormCure for recommended curing time and remove supports after this stage. Peel the supports from the model by hand for larger areas which are easy to access. To remove supports from tight areas within the model it is best to use forceps or tweezers.



When all supports have been successfully removed, wipe over the model with a microfiber cloth and IPA to remove any excess tackiness.

An air compressor may also be used to remove debris when required.

14.5.1.3. Post curing prints using a Form Cure

Post-curing enables parts to reach the highest possible strength and become more stable. Post-curing is particularly important for Formlabs' range of functional resins: Castable, Flexible and Tough. After printing, optimizing the strength of parts depends on light and heat. Post-curing at higher temperatures results in a shorter time to fully cure. Additionally, higher temperatures lead to higher mechanical properties.



Optimal post-curing settings depend on equipment and the geometry of the part.

Ensure the parts to be cured are fully dry and have no solvent trapped on surfaces or interior of the part. Curing parts that contain solvent can dissolve resin inside the part and prevent parts from strengthening to their material properties.

Open the FormCure hood and distribute parts to be cured onto the round turntable. Close hood to allow part to begin curing.

Turn knob to navigate the display menu and set the material type and version to see the recommended Form Cure time and temperature settings. This will automatically adjust the Time and Temperature values.

These times are updated regularly so please check your resin's recommended post-cure time and temperature before beginning a post-cure cycle at www.formlabs.com.

You can manually adjust the time and temperature by selecting the Material value to Custom if required.



14.5.2. Form Cure material settings:

| Resin | Form Printer | Cure Time (min) | Temperature Notes (degrees) |
|-----------------|-------------------------|-----------------|---|
| White | 3 / 3B / 3L / 3BL | 30 | 60 Use these settings for standard opaque resins including Black, Grey, Color, and Model, which have equivalent mechanical properties. |
| Grey | 3 / 3B / 3L / 3BL | 30 | 60 Use these settings for standard opaque resins including Black, White, Color, and Model, which have equivalent mechanical properties. |
| Clear | 3 / 3B / 3L / 3BL | 15 | 60 |
| Flexible 80a | 3 / 3B / 3L / 3BL | 10 | 60 There is only one recommended post-curing time for Flexible 80A V1. |
| Clear v4.1 | 3 / 3B / 3L / 3BL | 15 | 60 - Optimal for clarity and strength - too much curing may lead to yellowing |

| | | | |
|-----------------|-------------|----|---|
| Biomed White | 3B / 3BL | 30 | 60 - Cycle ensures parts meet mechanical strength requirements |
| Biomed Clear | 3B / 3BL | 30 | 60 - Cycle ensures parts meet mechanical strength requirements |

14.5.3. Removing Support Bumps from 3D Models

If supports are still visible in certain internal areas, use the snips or tweezers to remove them. Use hand files to remove support marks. A dremel can also be carefully used to remove support bumps.



Sandpaper should be used to give a smooth finish.

NOTE: Gradually move from lower grade up to high grade as required. Metal filing tools can also be used in this step.



NOTE: Only remove the support bumps to ensure all landmarks are as close to exact as possible

Once the model has been completely filed, wash the model under tap water. Use a toothbrush to remove any trapped dust. Dry the model with a microfiber cloth and leave the model to dry further in a ventilated area.

Removing support touchpoints sometimes leaves raised marks and divots on the parts surface. To reduce these marks, begin by using metal hand files to remove larger support marks. Dremel's can also be used. Then use sandpaper to give a smooth finish. Begin by using the lowest grit sandpaper and gradually work to a higher sequence. Using a sequence of 240, 320, 1000 grit sandpaper.

NOTE: When sanding clear models, this procedure must be repeated until the clear model has a glass finish. Wet sanding paper to reduce dust and create a finer surface finish. Wet the surface of the model and sand down.

Use a squirt bottle to rinse the part with IPA or water and use a toothbrush to remove dust caused by sanding. Leave to dry before proceeding with the stage of post-production.

14.6. HP post-processing of 3D printed models

Remove the build unit from the printer after printing the parts.

Allow models to cool for the recommended time based on volume.

| Build chamber | Printing time | | Safety cooling time | Natural cooling time | | Fast cooling time * |
|---------------|-----------------|-----------------------------|---------------------|----------------------|-----------|---------------------|
| | Fast print mode | Default/Strength print mode | | Normal | Minimum * | |
| 100% full | 10 h | 16 h 20 min | 20–30 min | 46 h | 31 h | 10 h |
| 75% full | 7 h 30 min | 12 h 15 min | 20–30 min | 35 h | 23 h | 8 h |

| Build chamber | Printing time | | Safety cooling time | Natural cooling time | | Fast cooling time * |
|---------------|-----------------|-----------------------------|---------------------|----------------------|-----------|---------------------|
| | Fast print mode | Default/Strength print mode | | Normal | Minimum * | |
| 50% full | 5 h | 8 h 10 min | 20–30 min | 23 h | 16 h | 6.5 h |
| 25% full | 2 h 30 min | 4 h | 20–30 min | 12 h | 8 h | 5 h |

Once models have been cooled you must clean the parts to remove the thin layer of material attached to the surface.

To do this, you need a bead-blasting machine. HP recommends a bead-blasting machine with the following specification:

For PA materials:

- Manual or automatic operation
- Air pressure in the range 2–5 bar (29–72.5 psi)
- Glass beads of 70–110 µm diameter (0.00276–0.00433 in)

This process consists of shooting an abrasive media, usually a bead (size and type results in different surface finishes), at high pressure at a printed part with compressed air, knocking loose unfused powder while also smoothing the finish of the part.



14.7. Stratasys post-processing of 3D printed models on Polyjet technology

Remove the model from the build chamber.

Cleaning the Model

Using the WaterJet, remove the support material from the model as thoroughly as possible.



Immerse the model in the sodium hydroxide solution for up to two hours, depending on the model size and type.

Caution: Do not let sodium hydroxide come in contact with your eyes or skin. It may cause chemical burns, scarring and blindness. Use protective goggles and nitrile gloves when handling sodium hydroxide and models soaked in it. In case of direct contact with sodium hydroxide, clean the affected area immediately with running water and seek medical attention. Mixing sodium hydroxide with water generates heat that could ignite other materials.

Remove the model from the solution and immediately rinse the model under running tap water.

Using the WaterJet, remove any remaining support material from the model.

Wipe down the model with a disposable paper towel and wait until the model is completely dry. (For faster drying, immerse the model in isopropyl for a few seconds and let the model dry for at least half an hour)

14.8. Stratasys post-processing of 3D printed models on DLP technology

- Remove the build plate with the model from the printer.




- Detach the 3D printed model from the build plate.
- Remove printed supports from the model by hand or with Snips.
- Clean the parts by soaking them in a solution of IPA in an ultrasonic bath, place the part in a container of IPA solution and place in an ultrasonic bath for 2 minutes.
- Remove the part from the IPA solution and place into a second container of IPA solution, place in the ultrasonic bath for a further 2 minutes.
- Wipe the model clean and air dry for 2-3 hours depending on the size of the part
- Place the part in the Dymax ECE5000 UV Cure
- Press the curing button and cure the model for:
 - o Small models: 2 minutes turning every 30 seconds.
 - o Large models: 6- 8 minutes turning every 30 seconds.
- The part will need to be rotated during the cure process to ensure all sides are fully cured.
- Sand down any support bumps using 600 grit sandpaper.




14.9. Final inspection of the 3D printed model

All digital files provided by Axial3D have a calibration token applied to the anatomical model. This calibration token measures 10 mm x 10 mm. On completion of post-processing the 3D printed anatomical model the end user should carry out a calibration inspection using calibrated digital vernier calipers.

Overall visual inspection shall be carried out to confirm the finish quality of the 3D printed model.

15. Symbols glossary

| Symbol | Title | Standard Designation Number | Description of Symbol |
|---|---|---|--|
|  | Batch code | ISO 15223-1:2016 (new draft in review) (Symbol 5.1.5) Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied | Indicates the manufacturer's batch code so that the batch or lot can be identified. |
|  | Medical Device | ISO 15223-1:2019 (new draft in review includes this symbol) (Symbol 5.7.4) Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied | Indicates the item is a medical device |
| Desc. | Product description | N/A | N/A |
|  | Consult instructions for use or consult electronic instructions for | ISO 15223-1:2016 (new draft in review) (Symbol 5.4.3) Medical devices - Symbols to be used with medical device labels, labelling and | Indicates the need for the user to consult the instructions for use. NOTE 1 Synonym for "Consult instructions for use" |

| | | | |
|---|---------------------|--|---|
| | use | information to be supplied | is "Consult operating instructions". |
|  | Manufacturer | ISO 15223-1:2016 (new draft in review) (Symbol 5.1.1) Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied | Indicates the medical device manufacturer. Can be used with ISO 8601 date of manufacturer, YYYY-MM-DD |
|  | Caution | ISO 15223-1:2016 (new draft in review) (Symbol 5.4.4) Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied | To indicate that caution is necessary when operating the device or control close to where the symbol is placed, or to indicate that the current situation needs operator awareness or operator action in order to avoid undesirable consequences. |
|  | Date of manufacture | ISO 15223-1:2016 (new draft in review) (Symbol 5.1.3) Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied | Indicates the date when the medical device was manufactured. To be used with ISO 8601 date of manufacturer, YYYY-MM-DD |

| | | | |
|---|----------------------------------|---|---|
|  | <p>Fragile, handle with care</p> | <p>SO, 15223-1:2016 (new draft in review) (Symbol 5.3.1) Medical devices - Symbols to be used with medical device labels, labelling and information to be supplied</p> | <p>Indicates a medical device that can be broken or damaged if not handled carefully.</p> |
|  | <p>Prescription Only</p> | <p>CFR 21 801.15(c)(1)(i)(F) (US FDA) Labelling - Medical device: Prominence of required label statements CFR 21 801.109 (US FDA) Labelling - Prescription Devices</p> | <p>Requires a prescription in the United States of America Caution: Federal (USA) law restricts this device to sale by or on the order of a physician.</p> |

16. Manufacturer details



Axial Medical Printing Limited
17A Alexander House Ormeau Avenue
Belfast, BT2 8HD
+44 (0)2890 183590 (UK)
+1 857 412 7244 (US)

17. Reporting to adverse events to the FDA

MedWatch is the Food and Drug Administration's (FDA) program for reporting serious reactions, product quality problems, therapeutic inequivalence/failure, and product use errors with human medical products, including drugs, biologic products, medical devices, dietary supplements, infant formula, and cosmetics.

If you think you or someone in your family has experienced a serious reaction to a medical product, you are encouraged to take the reporting form to your doctor. Your health care provider can provide clinical information based on your medical record that can help the FDA evaluate your report.

However, we understand that for a variety of reasons, you may not wish to have the form filled out by your healthcare provider, or your health care provider may choose not to complete the form. Your health care provider is not required to report to the FDA. In these situations, you may complete the Online Reporting Form yourself.

You will receive an acknowledgement from the FDA when your report is received. Reports are reviewed by FDA staff. You will be personally contacted only if we need additional information.

Submitting Adverse Event Reports to FDA

Use one of the methods below to submit voluntary adverse event reports to the FDA:

Report Online at:

www.accessdata.fda.gov/scripts/medwatch/index.cfm?action=reporting.home



Consumer Reporting Form FDA 3500B. Follow the instructions on the form to either fax or mail it in for submission. For help filling out the form, see MedWatchLearn.

The form is available at

www.fda.gov/downloads/aboutFDA/reportsmanualsforms/forms/ucm349464.pdf

Call FDA at 1-800-FDA-1088 to report by telephone.

Reporting Form FDA 3500 commonly used by health professionals. The form is available at

www.fda.gov/downloads/aboutFDA/reportmanualsforms/forms/ucm163919.pdf

18. Glossary

| Terminology/ Abbreviations/ Acronyms/ Definitions | Meaning |
|---|---|
| Bead-Blasting | The operation of propelling, typically with compressed air, a stream of abrasive material against a surface to affect the surface finish. |
| Build Platform/Build Plate | The plate will hold the 3D print and move layer by layer as the model is made |
| CAD | Computer Aided Design |
| Calibration Token | A small additional part of known dimensions added as part of the QA process to ensure accurate printing. |
| Cardiovascular | relating to the heart and blood vessels. |
| CT | Computed Tomography |
| DICOM | Digital Imaging and Communications in Medicine |
| Digital Vernier Calipers | A precision instrument that can be used to measure |

| | |
|-----------|--|
| | internal and external distances extremely accurately |
| DLP | DLP (Digital Light Processing) is a 3D printing technology used to rapidly produce photopolymer parts. |
| Form Cure | Used to post-cure 3D printed models |
| Form Wash | Used to wash 3D printed models in IPA after printing |
| In-Situ | In the natural or original position or place |
| IPA | Isopropyl alcohol |
| NM | Nuclear Medicine |
| OBJ | It is a file format used for a three-dimensional object containing 3D coordinates (polygon lines and points), texture maps, and other object information |
| Ortho | Orthopaedic |
| PACS | Picture archiving and communication system |
| Pathology | The structural and functional deviations from the normal that constitute disease or characterize a particular disease |

| | |
|-----------------|--|
| Post-Processing | The process of removing a printed model from a printer and applying finishes to create the final product |
| PPE | Personal Protective Equipment |
| Pre-Processing | The process of making a 3D file ready for printing through addition of dowels and branding |
| Raft | A horizontal latticework of filament that is located underneath your part, to support the 3D print process |
| Resin | UV curing liquid used as the substrate for printing |
| Segmentation | The process of labelling 2D images |
| STL | Describe only the surface geometry of a three-dimensional object without any representation of color, texture or other common CAD model attributes |
| Support Bumps | Small, raised areas on the print surface caused by the removal of supports |
| Supports | Disposable thin lattice structures automatically added to assist in supporting a 3D printed model |

| | |
|--------------|---|
| Surfaces | 3D models of the 2D labels that can be exported |
| Surface view | The function used to view the generated surface as a 3D model for export |
| Tank | A resin tank with a transparent base and non-stick surface, which serves as a substrate for the liquid resin to cure against, allowing for the gentle detachment of newly formed layers |
| Topology | The anatomical structure of a specific area or part of the body |
| UV | Ultra-violet |
| WaterJet | A stream of water forced out through a small aperture |
| 3D mesh | Is a collection of vertices, edges and groups to produce a 3D model |
| 3MF | 3D manufacturing format file type |

19. Appendix Axial3D Insight Release Notes v2.0.0

19.1. Known Software Anomalies

The Axial3D Insight Release Notes v2.0.0 provided alongside this Operator Manual can be referenced to inform the end user of any known issues or anomalies.

Any issues or anomalies present a negligible risk to the end user and this appendix details any actions that should be taken by the end user upon encountering such an anomaly.

Approved By:
[\(CO-149\) Insight Redesign 2.0](#)

Description

CO required to capture all of the changes for the Insight Redesign 2.0.0 update/.

Justification

CO required to capture all of the changes for the Insight Redesign 2.0.0 update/.

| Assigned To: | Initiated By: | Priority: | Impact: |
|-------------------|-------------------|-----------|---------|
| Noeleen McCullagh | Noeleen McCullagh | High | Major |

Version History:

| Author | Effective Date | CO# | Ver. | Status |
|----------------|-----------------------------|------------------------|------|------------|
| Cathy Coomber | August 21, 2025 3:33 PM GMT | CO-149 | 2 | Published |
| Cathy Coomber | July 23, 2025 8:22 AM GMT | CO-145 | 1 | Superseded |
| Neisha Kearney | August 19, 2024 4:00 PM GMT | CO-62 | 0 | Superseded |